

# DEVELOPMENT OF AN ELECTROLABIOPHOTOGRAPH EMBEDDED IN A TROMBONE MOUTHPIECE FOR THE STUDY OF LIP OSCILLATION MECHANISMS IN BRASS INSTRUMENT PERFORMANCE

Vincent Freour and Gary Scavone

Computational Acoustic Modeling Laboratory, Centre for Interdisciplinary Research in Music Media and Technology, Schulich School of Music, McGill University, Montréal, Québec, Canada.

## 1. INTRODUCTION

The lips of a brass instrument player constitute a complex pressure-controlled valve from which the vibration of the air column originates. Due to their anatomical properties and the significant ability from the player to control their geometry and mechanical characteristics, the behavior of lip valves has been a growing subject of interest. In order to investigate lip mechanics on real players, different in-vivo methods have been proposed. Lip opening area and frequency response have been evaluated on real players using high speed imaging [1]. This technique requires the use of special transparent mouthpieces with cylindrical cup that allows un-distorted image captures but may significantly affect the behavior of the lips. Lip vibratory mechanisms have been investigated using strain gauges located between the lips and the mouthpiece rim [2]. This solution remains however quite invasive since the strain gauge is usually attached to the upper lip of the subject. Experiments have also been conducted on artificial lip systems which allow the use of highly intrusive measurement devices such as laser velocimetry or light transmission and video methods [1,3]. However, although artificial lips are becoming more and more accurate in reproducing brass instruments sounds, they are still approximations of human lips and have not proven their ability yet in reproducing human players' behaviour over the all playing range of a trumpet or a trombone.

In this paper, we present a method for the investigation of lip motion in trombone players based on the measurement of lip conductivity. In the scope of this study, experimental data are evaluated regarding the phase relationship between the lip displacement and the acoustic pressure in the mouthpiece. This phase information provides knowledge about the predominant "outward" or "upward" striking characteristic of the valve as proposed in [4]. Results are compared to previous recordings obtained using other measurement techniques, as well as numerical simulations.

## 2. METHODS

### 2.1 Development of an electrolabiograph

For the purpose of in-vivo investigations on brass players' lips we developed an electrolabiograph (ELG) based on the principle electroglottography (EGG) as firstly presented by Fabre in 1956 [5]. Analogously to the EGG for the study of vocal folds contact, the ELG records the variations of electrical admittance between two electrodes

by mean of a high frequency modulated current sent through the lips. The two electrodes are located across the lips (one electrode on the upper lip and one on the lower lip). Therefore, the ELG signal is assumed to be proportional to the degree of contact of the lips.

In order to reduce the intrusiveness of the system, the contact electrodes were made tin-plated copper foil shielding tape glued on the mouthpiece rim. The resistance of the electrode pair was raised to  $40\Omega$  by a resistor soldered to one of the electrodes in order to fit with the signal conditioner requirements. Electrodes were connected to a commercial Voce Vista EGG signal conditioner. And the analog output sent to a National Instrument converter. This system is therefore totally non-invasive, the only restriction relying on the use of non conductive material mouthpiece. In this study, we use a plastic mouthpiece designed by CFMI Université Lille 3 in France.

### 2.2 Determination of the valve mechanism


Since ELG amplitude is proportional to the degree of contact between the lips, when the ELG amplitude decreases, the contact area at the lip interface decreases and the lips tend to open. Therefore, we can reasonably assume that the ELG and lip motion  $G$  are  $\pi$  out of phase, lip motion being defined as the distance between the center of mass of the two lips. Consequently, the inverse of the ELG signal is assumed to be in phase with the lip motion and thus in phase with the lip opening area  $S_{lip}$ :  $\varphi(-ELG) = \varphi(G) = \varphi(S_{lip})$ .

The predominant "outward" or "upward" striking mechanism of the lips is given by the sign of the phase difference between lip motion and the acoustic pressure measured in the mouthpiece cup by an Endevco 8510B-1 microphone. In the case of a positive phase difference, lip motion anticipates the drop of mouthpiece pressure so the lips behave as an "outward" striking valve. If the phase difference is negative, the pressure drop occurs before the lips tend to open so the lips behave as an "upward" striking valve.


## 3. EXPERIMENTS AND RESULTS

Experiments were conducted on one subject on a King 2102 tenor trombone. Figure 1 shows the results obtained for an overtone series from F3 to D5 and back to D5 in the closed position of the slide. The top graphic represents the waveform of the downstream pressure and ELG signal. The bottom graphic represents the phase difference between the

inverse of the ELG signal and the downstream pressure calculated on a 512 samples sliding window with 448 samples overlap.

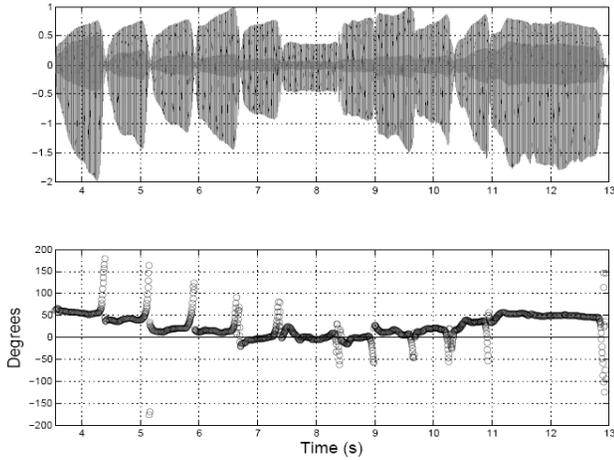

**Figure 1. Top: downstream pressure (lighter line), inverse of the ELG signal (darker line). Bottom: phase difference between green and blue waveforms.**

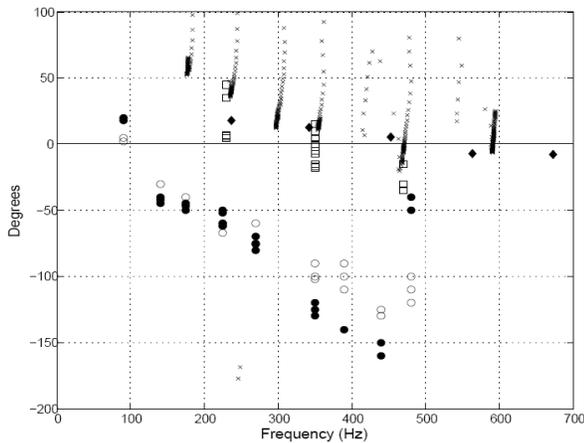

**Figure 1. Phase difference between lip motion and downstream pressure in French horn (filled and empty circles), trumpet (empty squares), numerical simulation of trumpet (diamonds) and trombone (crosses).**

The maximum phase difference is observed for the lower tone (F3) around 50 degrees and reveals a clear “outward” striking behaviour of the reed. The minimum value occurs for B4flat and D5 for which the phase difference is near 0. Therefore, the tendency of a transition from an “outward” to an “upward” striking regime of oscillation is confirmed on this acquisition.

The phase data presented on Figure 1 is now plotted against the playing frequency on Figure 2. On the same graphic we represent the phase difference between lip motion and downstream pressure in French horn and trumpet measured on real player by Yoshikawa using strain

gauges [2]. The phase difference between lip opening area and downstream pressure in trumpet obtained from numerical simulations by Adachi and Sato [6] is also plotted on the same figure. Results from simulations and in-vivo measurements in trumpet are quite consistent, which suggests good performances from the two-dimensional lip model proposed by Adachi and Sato. Phase values obtained in French horn are clearly lower than the one obtained for trombone and trumpet, possibility because of the specific geometry of the French horn bore and mouthpiece (conical bore). Results obtained for the trombone in this study are consistent with the tendency observed in previous studies with an order of magnitude close to values observed in trumpet.

#### 4. DISCUSSION AND CONCLUSIONS

We have presented a new sensor for the measurement of lip electrical admittance in trombone performance. This method is totally non invasive and provides a signal which is assumed to be proportional to the degree of contact of the lips. Moreover, the phase of this signal is robust to the phase of the lip motion and opening surface, which allows to evaluate lip vibratory mechanism on real players, across various playing conditions. The results revealed a tendency to a transition from an outward striking to an upward striking regime of oscillation as expected from previous studies.

Although the scope of this paper is restricted to considerations on the phases of the signals, the ELG waveform displays some common features with EGG signals of the vocal folds. Therefore, some techniques for the extraction of additional information such as open quotient should be applied for further investigation. Correlations between ELG features and vocal-tract influence performed by measuring simultaneously the upstream and downstream pressure are also part of future works.

#### REFERENCES

- [1] M. J. Newton, M. Campbell, J. Gilbert: Mechanical response measurements of real and artificial brass players lips. *J. Acoust. Soc. Am.* **123**(1) (2008).
- [2] S. Yoshikawa: Acoustical behaviour of brass player’s lips. *J. Acoust. Soc. Am.* **97**(3) (1995), 1929-1939.
- [3] J. Gilbert, S. Ponthus, J-F Petiot: Artificial buzzing lips and brass instruments: Experimental results. *J. Acoust. Soc. Am.* **104**(3) (1998), 1627-1632.
- [4] N. H. Fletcher: Autonomous vibration of simple pressure-controlled valves in gas flows. *J. Acoust. Soc. Am.* **93**(4) (1993), 2172-2180.
- [5] P. Fabre: Un procédé électrique percutané d’inscription de l’accolement glottique au cours de la phonation : Glottographie de haute fréquence. *Bulletin de l’Académie Nationale de Médecine* (1957), 66-69.
- [6] S. Adachi, M. Sato: Trumpet sound simulation using a two-dimensional lip vibration model. *J. Acoust. Soc. Am.* **99**(2) (1996), 1200-1209.